




3034 DK - Homocysteine

Udsendelse 1 - 2016. Laboratorie nr. 191, resultat id. 191

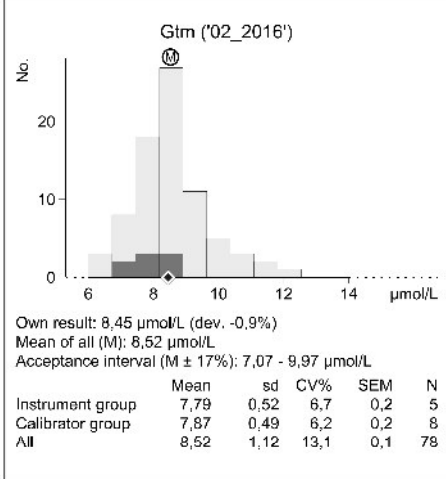


P-Homocystein; stofk. Calibrator: In-house - API 4000 LC/MS/MS
 Instrument group: LC-MS/MS Calibrator group: In-house

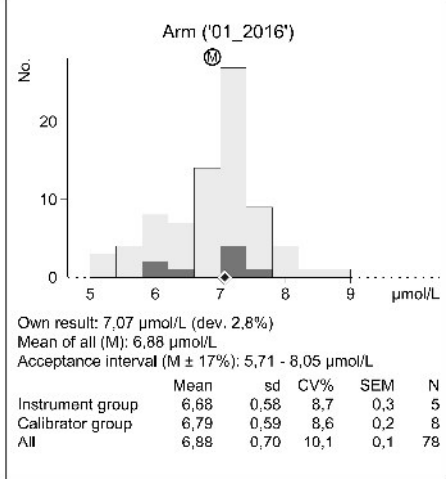

History

Round	Material	Target	Own	%dif	-17%	17%
16/01	Arm	6,88	7,07	2,8		
16/01	Gtm	8,52	8,45	-0,9		
15/05	Asm	12,68	12,8	1,0		
15/05	Hgc	17,19	17,1	-0,5		
15/04	Iqm	51,37	51,7	0,6		
15/04	Asm	12,79	11,4	-10,9		
15/03	Asm	12,77	13,5	5,7		
15/03	Arm	6,89	7,11	3,2		
15/02	Arm	6,65	6,0	-9,8		
15/02	Hgc	16,79	15,7	-6,5		
15/01	Hgc	16,98	16	-5,8		
15/01	Iqm	49,97	52	4,1		

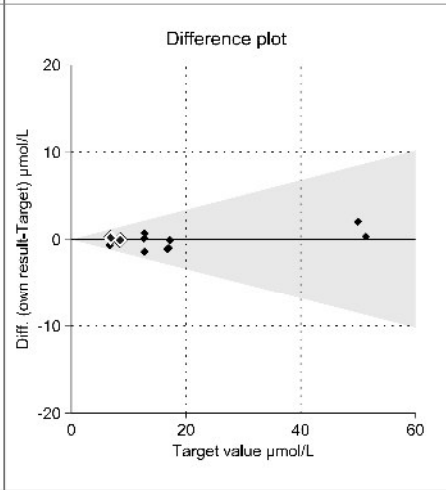

History for Arm

Round	Target	Own	%dif	-17%	17%
16/01	6,88	7,07	2,8		
15/03	6,89	7,11	3,2		
15/02	6,65	6,0	-9,8		

History for Gtm

Round	Target	Own	%dif	-17%	17%
16/01	8,52	8,45	-0,9		