

Analyte: Perphenazine

Results


Sample	Method	Result	Unit	Perf Score	Score Type	% Diff
PS16	LCMS & MS/MS	18.80	µg/L	0.01	zScore	0.27

Assessment Statistics

Sample	PS16
Assigned Value	18.75
Assigned Value Derived By	All data
Uncertainty of Assigned Value	0.434
SDPA	4.307
Satisfactory Range	10.14 to 27.36
Satisfactory z/z score	90.0%
Questionable z/z score	10.0%
Unsatisfactory z/z score	0.0%

Result Statistics

Sample	PS16
Number of Results	20
Number of Excluded Results	0
Mean	18.48
Median	18.75
Standard Deviation	3.829
Robust SD	1.551

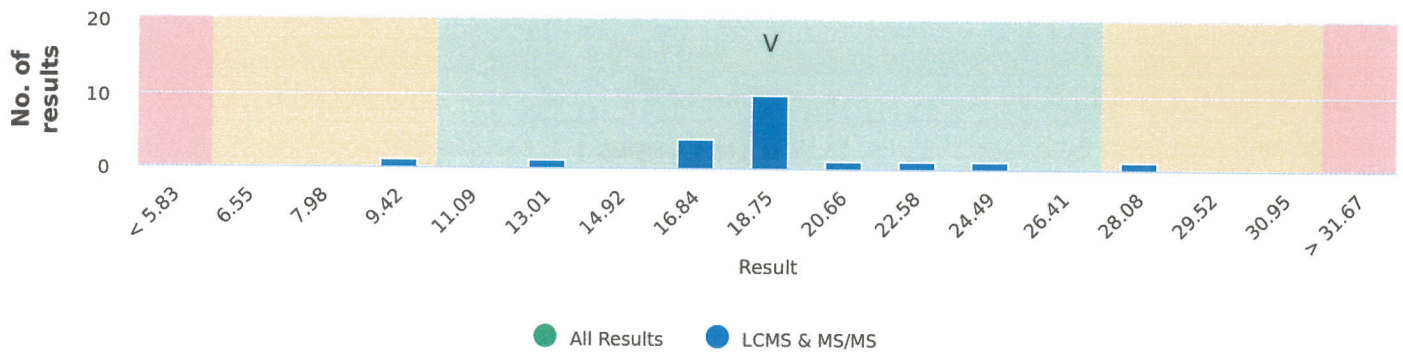

Last 9 Performance Scores

Sample PS16 - Round	194	197	200	203	206	209	212	215	218
LCMS & MS/MS		-0.39	-0.26	-0.82	-0.82	-0.10	-0.14	0.00	0.01

< or > = Less/Greater than result returned, no assessment given. ZS = Zero Spiked Sample, no assessment given. Blank = No result submitted

