


Distribution Number: 136
Date: Feb-16
Samples: Q3/135
Lab Number: 365

Serum - Free Kappa

Methods	n	Mean	SD	CV	<=>
Overall	266	7.862	1.10	14.0%	4
Binding Site FreeLite on BNI and ProSpec	66	7.751	1.16	15.0%	2
Binding Site FreeLite on Immage	26	8.665	0.60	6.9%	1
Binding Site FreeLite on Hitachi/Mod P	8	8.205	0.97	11.7%	0
Binding Site FreeLite on Beckman AU Series	13	7.405	0.92	12.5%	0
Binding Site FreeLite on ADVIA analysers	4	7.053	0.51	7.2%	0
Binding Site FreeLite on Integra 400/800	20	10.031	0.79	7.8%	0
Binding Site FreeLite on Roche c501/c502	34	8.571	0.75	8.8%	0
Binding Site SPAPLUS® FreeLite	97	7.799	0.71	9.1%	1
Miscellaneous	7	5.480	3.38	61.6%	0

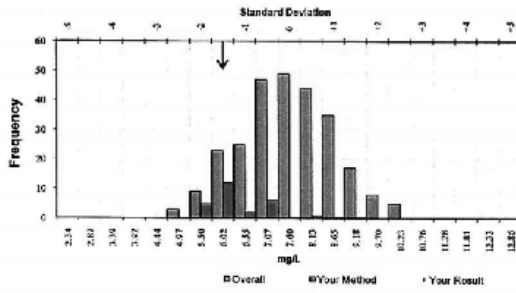

Overall Results

Bias	-21.8
BIS	-134
VIS	133.6
MRBIS	8.07
MRVIS	92.68


By Your Method

Bias	-5.71
BIS	-36.0
VIS	35.96
MRBIS	7.032
MRVIS	52.59

Your Result: 6.19
Binding Site FreeLite on Immage

Serum - Free Lambda

Methods	n	Mean	SD	CV	<=>
Overall	288	230.051	38.80	16.9%	0
Binding Site FreeLite on BNI and ProSpec	60	226.154	31.17	13.7%	0
Binding Site FreeLite on Immage	27	274.162	40.94	14.9%	0
Binding Site FreeLite on Hitachi/Mod P	6	234.577	21.53	9.2%	0
Binding Site FreeLite on Beckman AU Series	12	230.004	23.30	10.1%	0
Binding Site FreeLite on ADVIA analysers	4	226.923	16.93	7.4%	0
Binding Site FreeLite on Integra 400/800	20	296.899	16.23	5.4%	0
Binding Site FreeLite on Roche c501/c502	33	224.356	17.47	7.8%	0
Binding Site MININEPH PLUS FreeLite	1	236.700	0.00	0.0%	0
Binding Site SPAPLUS® FreeLite	57	216.365	36.09	16.6%	0
Miscellaneous	6	174.257	100.04	57.4%	0

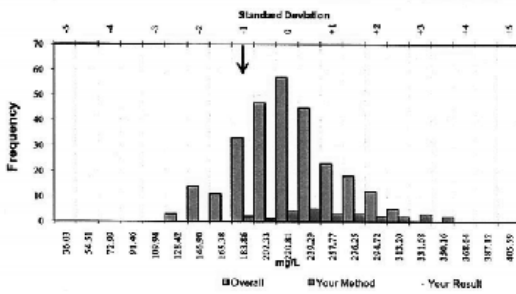

Overall Results

Bias	-19.3
BIS	-121
VIS	121.3
MRBIS	-29
MRVIS	63.8


By Your Method

Bias	-32.3
BIS	-200
VIS	202.0
MRBIS	-34.1
MRVIS	96.59

Your Result: 185.7
Binding Site FreeLite on Immage

Serum - Free Light Chain Ratio

Methods	n	Mean	SD	CV	<=>
Overall	270	0.036	0.01	24.5%	4
Binding Site FreeLite on BNI and ProSpec	68	0.036	0.01	26.5%	1
Binding Site FreeLite on Immage	26	0.026	0.01	21.7%	0
Binding Site FreeLite on Hitachi/Mod P	5	0.033	0.01	17.6%	0
Binding Site FreeLite on Beckman AU Series	12	0.036	0.00	12.5%	0
Binding Site FreeLite on ADVIA analysers	4	0.030	0.00	7.1%	0
Binding Site FreeLite on Integra 400/800	21	0.034	0.00	12.5%	0
Binding Site FreeLite on Roche c501/c502	30	0.039	0.00	11.4%	2
Binding Site MININEPH PLUS FreeLite	1	0.030	0.00	0.0%	0
Binding Site SPAPLUS® FreeLite	93	0.037	0.01	21.9%	1
Miscellaneous	8	0.030	0.01	23.6%	0

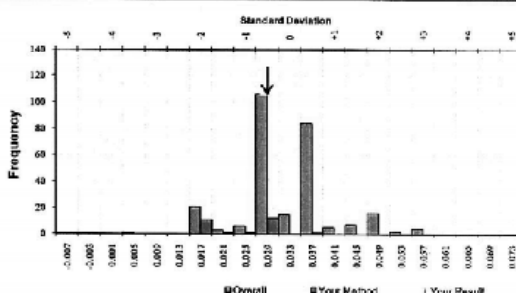

Overall Results

Bias	-13.6
BIS	-65.8
VIS	65.57
MRBIS	8.015
MRVIS	160.3

By Your Method

Bias	16.94
BIS	109.8
VIS	103.6
MRBIS	18.98
MRVIS	105.6

Your Result: 0.03
Binding Site FreeLite on Immage