


Analyt **Leukozyten**
Methode Alle Methoden

Erfolgsquote 96,3 %


Ausreisser 3

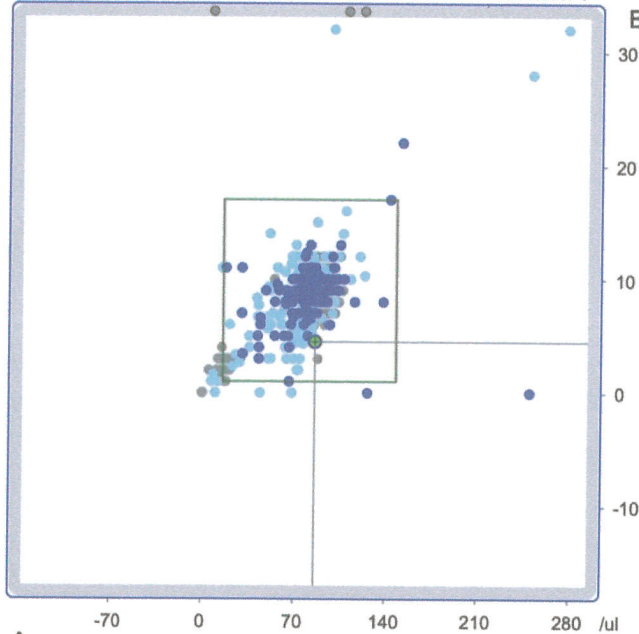

Teilnehmerzahl	649		
Probe/Einheit	A	/ul	B
Mittelwert	80.6		8.47
Standardabweichung	26.2		3.09
Variationskoeffizient	32.6		36.5


Probe A [ul]

M	Kit	N	Min	16.P	50.P	84.P	Max
Alle		649	0.089	65.0	87.0	97.0	278
1	89	13	41.3	54.3	84.0	99.0	120
1	91	123	18.0	64.3	80.0	94.0	250
1	92	40	7.00	29.2	67.8	87.0	107
1	93	11	25.7	42.5	73.0	82.2	82.6
1	95	32	42.0	64.1	78.3	87.9	124
1	96	35	52.0	63.6	77.3	86.3	95.6
1	97	11	23.0	52.4	77.0	90.3	94.0
1	99	25	28.3	58.0	80.0	98.4	109
2	63	10	90.0	90.8	93.5	96.7	99.0
2	64	52	0.095	86.5	93.0	98.5	104
3	64	24	81.0	87.0	94.5	99.0	105
6	63	28	73.0	86.0	95.0	96.4	101
6	64	163	0.089	83.0	92.0	97.0	107
6	75	31	11.0	14.0	17.0	19.3	88.0

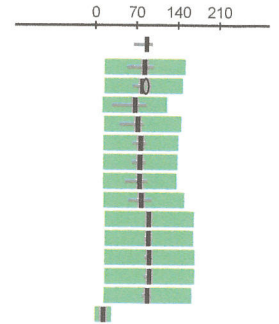

Probe B [ul]

M	Kit	N	Min	16.P	50.P	84.P	Max
Alle		649	0	6.60	9.00	10.3	87.0
1	89	13	6.00	7.24	8.10	10.8	12.0
1	91	123	0	6.58	9.00	10.3	22.0
1	92	40	0	4.12	8.00	11.4	15.0
1	93	11	0	3.07	7.67	11.2	11.3
1	95	32	3.00	5.76	8.33	11.0	12.0
1	96	35	2.00	5.25	8.50	10.1	12.0
1	97	11	2.33	6.32	9.00	10.6	12.0
1	99	25	2.67	7.16	9.00	11.0	32.0
2	63	10	8.00	8.00	9.00	10.0	10.0
2	64	52	0.011	8.00	9.00	10.0	87.0
3	64	24	7.00	8.00	9.00	10.0	11.0
6	63	28	7.00	7.64	9.00	10.4	12.0
6	64	163	0.009	8.00	9.00	10.0	12.0
6	75	31	1.00	1.41	2.00	3.00	4.00

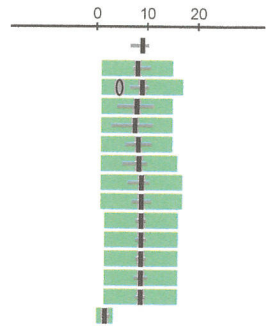


Die Abweichung Ihrer Ergebnisse vom Median des zugehörigen Unterkollektives (Kit) beträgt: A 7.1 % B -49.89 %

Andere Kits (Anzahl):
1-10(1), 1-84(2), 1-94(2), 1-98(2), 2-75(1), 2-77(5), 3-22(1), 3-63(4), 3-77(5), 3-91(2), 6-27(1), 6-67(1), 6-71(1), 6-74(5), 6-77(6), 6-79(5), 6-97(1), 6-99(2), 9-10(1), 9-22(1), 9-64(1), 9-95(1),

Analyt **Erythrozyten**
Methode Alle Methoden

Erfolgsquote 92,9 %


Ausreisser 4

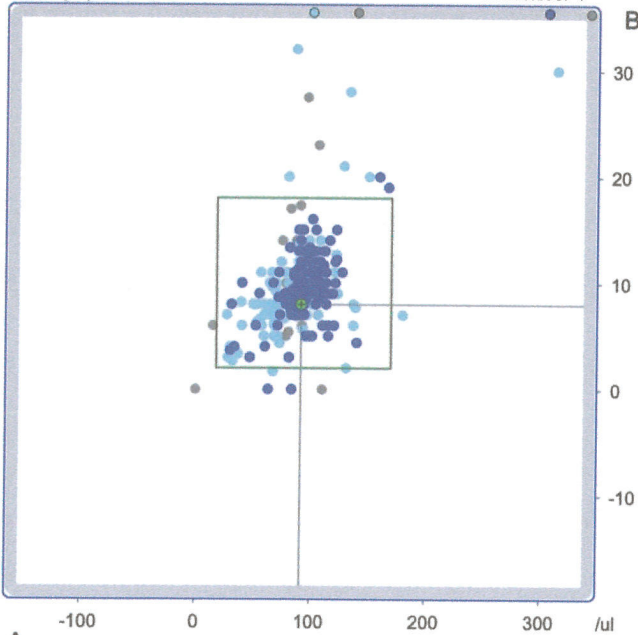

Teilnehmerzahl	314		
Probe/Einheit	A	/ul	B
Mittelwert	90.4		9.68
Standardabweichung	26.1		3.96
Variationskoeffizient	28.9		41.0


Probe A [ul]

M	Kit	N	Min	16.P	50.P	84.P	Max
Alle		314	0	71.8	92.0	107	2000
1	89	11	56.3	58.5	78.0	152	180
1	91	161	0	81.9	94.0	108	305
1	92	27	27.0	39.6	89.0	101	139
1	93	11	29.7	54.8	69.3	98.8	131
1	95	19	50.0	60.1	74.0	100	123
1	96	8	53.3	65.1	88.8	97.5	101
1	97	7	67.0		82.0		100
1	99	22	32.0	63.8	90.9	108	137
6	75	31	75.0	79.2	92.0	103	139
6	79	3	93.0		110		110



Probe B [ul]

M	Kit	N	Min	16.P	50.P	84.P	Max
Alle		314	0	7.00	9.37	12.0	2000
1	89	11	6.67	6.97	10.0	20.6	28.0
1	91	161	0	7.00	9.67	12.0	35.0
1	92	27	3.00	6.79	8.67	11.8	20.0
1	93	11	2.00	3.84	7.00	10.9	11.0
1	95	19	5.00	6.47	7.67	11.6	100
1	96	8	5.67	6.69	9.50	10.9	11.0
1	97	7	1.67		8.33		12.0
1	99	22	2.67	6.36	11.0	14.0	32.0
6	75	31	5.00	9.00	10.0	13.9	53.0
6	79	3	0		9.00		11.0



Die Abweichung Ihrer Ergebnisse vom Median des zugehörigen Unterkollektives (Kit) beträgt: A -2.8 % B -17.34 %

Andere Kits (Anzahl):
1-10(1), 1-88(1), 1-94(1), 1-98(2), 2-75(1), 3-75(1), 6-27(1), 6-71(1), 6-99(1), 9-22(1), 9-95(1), 9-99(2),